


CS6102 High Voltage Galvanic Stimulator Kit Quick Start Guide

The CS6102 kit includes the items shown in Figure 1.








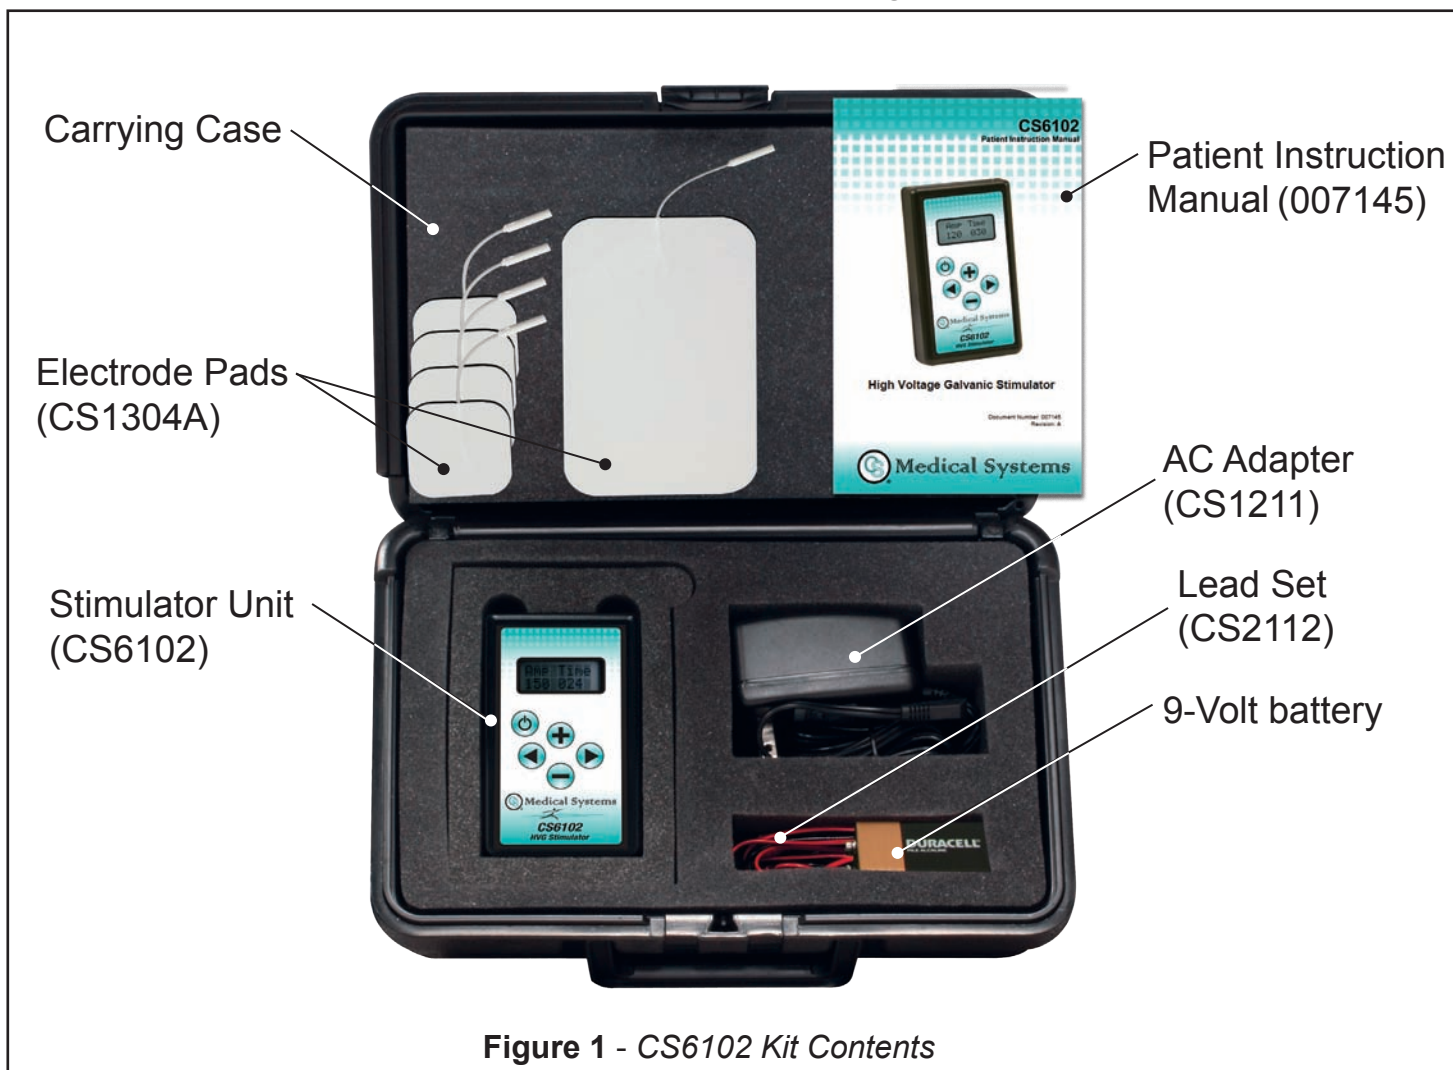




Once you have verified the kit contents, you can follow the steps to begin using your High Voltage Galvanic Stimulator.

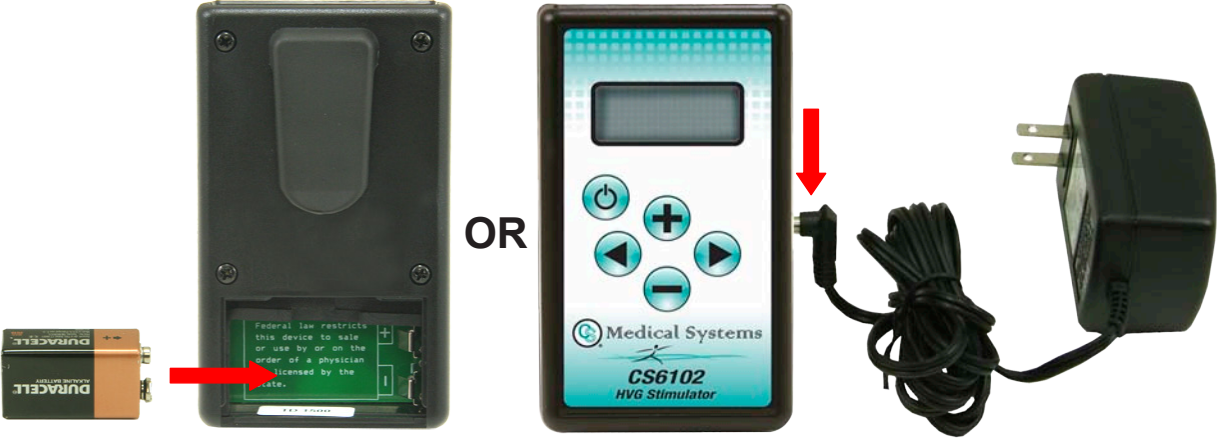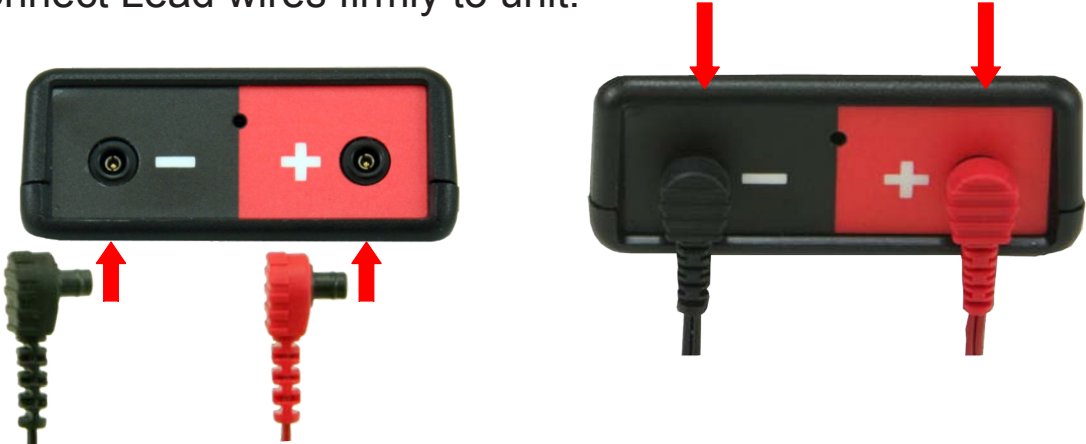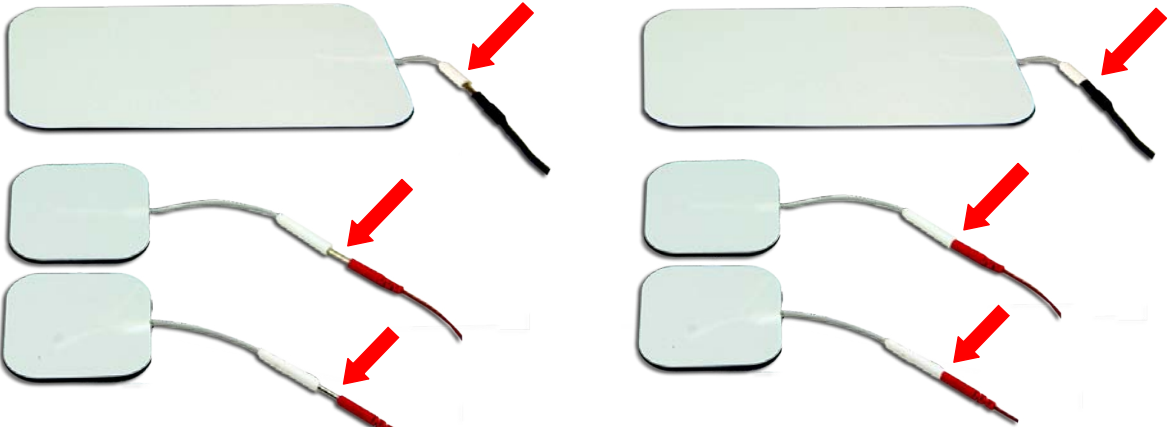







Operating details can be found in the CS6102 Patient Instruction Manual, document number 007145, which is included as part of the kit.

Document Number: 007286
Revision: A

| Step | Action |
|------|--|
| 1 | <p>Power:</p> <ul style="list-style-type: none"> - Provided by a 9-volt battery, or - Plugging the AC Adapter into the unit and an AC receptacle.  |
| 2 | <p>Connect Lead wires firmly to unit.</p>  |
| 3 | <p>Connect the Lead wires to Electrodes and place Electrodes per directions of healthcare provider.</p>  |

| Step | Action | | | | | | | | | | | | | | | | |
|-------------------|--|------|----------------|---------------|------------|-----------------|------------|------------------|------------|-------------------|------------|---------------|--------------|---------------|--------------|---------------|--------------|
| 4 | Press  to turn on stimulator.  | | | | | | | | | | | | | | | | |
| 5 | Press  to move to Mod (mode) field.  | | | | | | | | | | | | | | | | |
| 6 | Press  or  to select the mode of operation prescribed by healthcare provider. Modes are: DAY-NGT-FSP-MSP-M1-M2-M3. <table border="1" data-bbox="300 1440 989 1801"> <thead> <tr> <th>Mode</th> <th>Treatment Time</th> </tr> </thead> <tbody> <tr> <td>DAY - Daytime</td> <td>30 minutes</td> </tr> <tr> <td>NGT - Nighttime</td> <td>30 minutes</td> </tr> <tr> <td>FSP - Full Sweep</td> <td>30 minutes</td> </tr> <tr> <td>MSP - Muscle Pump</td> <td>20 minutes</td> </tr> <tr> <td>M1 - Memory 1</td> <td>Programmable</td> </tr> <tr> <td>M2 - Memory 2</td> <td>Programmable</td> </tr> <tr> <td>M3 - Memory 3</td> <td>Programmable</td> </tr> </tbody> </table>  | Mode | Treatment Time | DAY - Daytime | 30 minutes | NGT - Nighttime | 30 minutes | FSP - Full Sweep | 30 minutes | MSP - Muscle Pump | 20 minutes | M1 - Memory 1 | Programmable | M2 - Memory 2 | Programmable | M3 - Memory 3 | Programmable |
| Mode | Treatment Time | | | | | | | | | | | | | | | | |
| DAY - Daytime | 30 minutes | | | | | | | | | | | | | | | | |
| NGT - Nighttime | 30 minutes | | | | | | | | | | | | | | | | |
| FSP - Full Sweep | 30 minutes | | | | | | | | | | | | | | | | |
| MSP - Muscle Pump | 20 minutes | | | | | | | | | | | | | | | | |
| M1 - Memory 1 | Programmable | | | | | | | | | | | | | | | | |
| M2 - Memory 2 | Programmable | | | | | | | | | | | | | | | | |
| M3 - Memory 3 | Programmable | | | | | | | | | | | | | | | | |

| Step | Action |
|------|--|
| 7 | Press  to move to the amplitude (Amp) field.  |
| 8 | Press  or  to set the Amp value prescribed by healthcare provider. <div style="border: 1px solid black; padding: 5px; display: inline-block;">  If the Amp value is zero (0), the unit will not begin treatment. </div>  |
| 9 | Treatment will begin after the stimulator is idle for approximately 10 seconds. |
| 10 | The face of the stimulator will display the Amp value and count-down timer. <div style="border: 1px solid black; padding: 10px; margin: 10px auto; width: fit-content;"> <p style="text-align: center;">AMP Time 150 020</p> </div> |
| 11 | Treatment ends when timer reaches zero (0). |
| 12 | The unit will power off after 5 minutes. |
| 13 | When complete, carefully remove lead wires and electrodes. |
| 14 | Place the unit and all accessories in the provided carrying case. |